

CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Laboratory Number:

Report Issue Date:

Order Date:

Analysis Date:

Sample Description:



Extraction Technician: LL

Analytical Chemist: LL

Unit Weight:

Laboratory Manager

CANNABINOID PROFILE- EXPANDED

Analyte	LOQ (mg/g)	Results	%
---------	------------	---------	---

Analyte	LOQ (mg/g)	Results	%
---------	------------	---------	---

Analyte	LOQ (mg/g)	Results	%
---------	------------	---------	---

Max Active THC

Total Active Cannabinoids

Max Active CBD

Total Cannabinoids

Cannabidiol(CBD) Cannabidivarin(CBDV) Cannabidiolic Acid(CBDA) Cannabigeronic Acid(CBGA) Cannabigerol(CBG) Cannabidiol(CBD)
 Tetrahydrocannabinol(THC) Tetrahydrocannabinolic Acid(THCA) Cannabinol(CBN) Delta-9-Tetrahydrocannabinol(D9-THC) Delta-8-Tetrahydrocannabinol(D8-THC)
 9S-Delta-10-Tetrahydrocannabinol(9S-D10-THC) 9R-Delta-10-Tetrahydrocannabinol(9R-D10-THC) 9S-Hexahydrocannabinol(9S-HHC) 9R-Hexahydrocannabinol(9R-HHC) 11-Hydroxy-THC (11-OH-D8-THC)
 Cannabichromene(CBC) Cannabichromenic Acid(CBCA) Tetrahydrocannabinolic Acid(THCA) Delta-9-Tetrahydrocannabinol(THC) Delta-8-Tetrahydrocannabinol-O-Acetate (D8-THCO) Tetrahydrocannabihexol (THCH)

Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.
 N/D: Not Detected LOQ: Limit of quantification

Analysis Method: ATL-LCM-001. Accurate Test Lab estimated expanded uncertainty is 13% as per in VALIDATION AND VERIFICATION OF ATL-LCM-001 (ATL-500A)



CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Laboratory Number:

Report Issue Date:

Order Date:


Analysis Date:

Sample Description:

Extraction Technician:LL

Analytical Chemist:LL

Unit Weight:

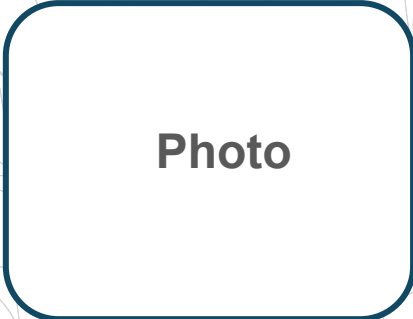

Kim Dang
Laboratory Manager

FILTH & FOREIGN MATERIALS PROFILE

Filth & Foreign Materials	% Detected by Weight	Allowable Criteria	PASS / FAIL
---------------------------	----------------------	--------------------	-------------

NOTES



Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC. ND:Not Detected - NA:Not Analyzed - CFU:Colony-forming unit / Analysis Method: ATL-PHI-001 / Accurate Test Lab estimated expanded uncertainty is less than 10% (Hogan, 2022). 1-Pass/Fail criteria based on CMTL sample testing Florida Department of Health Emergency Rule for 2020
Accurate Test Lab, LLC >>> 1305 NW 65th PI, Fort Lauderdale FL, 33309 USA.

>>> ☎ (954) 515 - 0200

CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Laboratory Number:

Report Issue Date:

Order Date:


Analysis Date:

Sample Description:

Extraction Technician:LL

Analytical Chemist:LL

Unit Weight:

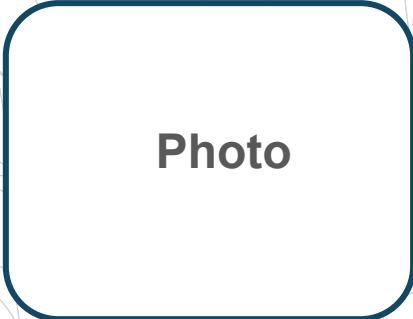

Kim Dang
Laboratory Manager

MICROBIOLOGY ANALYSIS

Microbe(s)	CFU Detected	Limit of Detection (CFU/g)	CFU/g	PASS / FAIL

NOTES



Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.
TNTC: Too numerous to count - ND: Not Detected - NA: NotApplicable -CFU: Colony-forming unit 1-Pass/Fail criteria based on CMTL sample testing Florida Department of Health Emergency Rule for 2020, Pass: Results within limits /specifications, Fail: Results exceed limits/specifications Accurate Test Lab estimated expanded uncertainty(CFU/g):-Aerobic Plate Count:10 -Staphylococcus Aureus:4 - Yeast:4 - Mold:2 - Enterobacteriaceae:6. Analysis Method: ATL-PHI-002

CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Laboratory Number:

Report Issue Date:

Order Date:


Analysis Date:

Sample Description:

Extraction Technician:AA

Analytical Chemist:AA

Unit Weight:

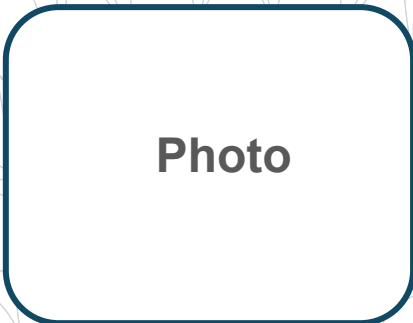

Kim Dang
Laboratory Manager

PESTICIDES PROFILE

Analyte	RESULT	PASS/FAIL	Analyte	RESULT	PASS/FAIL	Analyte	RESULT	PASS/FAIL
---------	--------	-----------	---------	--------	-----------	---------	--------	-----------

--	--	--	--	--	--	--	--	--

NOTES



Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC. N/D: Not Detected T:Trace Cannabinoids detected but are below limit of quantification.

1-California Code of Regulations, Title 16, Section 5719. ND: Not Detected - NT: Not Tested
Accurate Test Lab, LLC >>> 1305 NW 65th PI, Fort Lauderdale FL, 33309 USA.

>>> ☎ (954) 515 - 0200

CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Report Issue Date:

Order Date:

Laboratory Number:


Analysis Date:

Sample Description:

Extraction Technician:LL

Analytical Chemist:LL

Unit Weight:

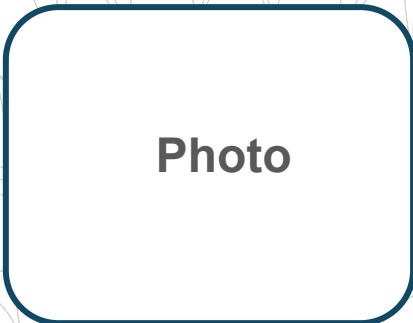

Kim Dang
Laboratory Manager

Salmonella spp - STEC E. coli - Aspergillus

Microbe

Detected /
absent

Action Limit

Pass / Fail

Microbe	Detected / absent	Action Limit	Pass / Fail

NOTES



Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.

NA= Not applicable ; ND= Not detected; NT: Not tested ; LOD= <10 CFUs ; qPCR LOD= <1 CFU/g - Method of Analysis qPCR PASS-FAIL; Criteria based on CMTL Sample Testing Florida Department of Health Emergency Rule for 2020

Accurate Test Lab, LLC >>> 1305 NW 65th PI, Fort Lauderdale FL, 33309 USA.

>>> (954) 515 - 0200

CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Laboratory Number:

Report Issue Date:

Order Date:


Analysis Date:

Sample Description:

Extraction Technician:AA

Analytical Chemist:AA

Unit Weight:

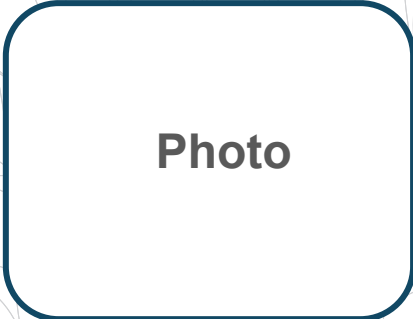

Kim Dang
Laboratory Manager

RESIDUAL SOLVENTS PROFILE

Analyte	Concentration (PPM)	Action Limit (PPM)	PASS/FAIL

NOTES



Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC.

N/D: Not Detected LOQ: Limit of quantification
Analysis Method: ATL-GCM-001
1-Pass/Fail statement is based on Florida Department of Health, Rule No 64ER-20-39. Accurate Test Lab estimated expanded uncertainty is 25%, Following NIST, EURACHEM & CITAC guidelines.

CERTIFICATE OF ANALYSIS



Customer:

Batch #:

Laboratory Number:

Report Issue Date:

Order Date:


Analysis Date:

Sample Description:

Extraction Technician:KD

Analytical Chemist: KD

Net Weight:

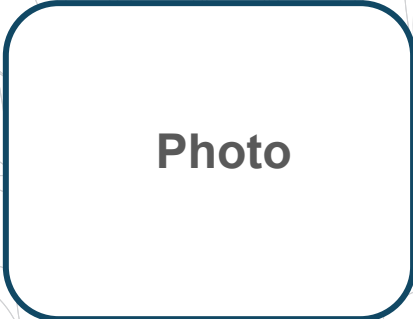

Kim Dang
Laboratory Manager

HEAVY METALS PROFILE

Analyte	LOD (ppb)	LOQ (ppb)	Action level (ppb)	Result (ppb)

NOTES



Reporting Limits will vary based on sample extraction weight used for the analysis. Accurate Test Lab, LLC utilizes based upon traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced. Results only apply to samples within COA as received. Certificate of Analysis shall not be reproduce except in full without approval of Accurate Test Lab, LLC. N/D: Not Detected Trace Cannabinoids detected but are below limit of quantification. LOQ = Limit of Quantitation, LOD = Limit of Detection, Dilution = Dilution Factor (ppb) = Parts per Billion,(%) = Percent, (cfu/g) = Colony Forming Unit per Gram(cfu/g) = Colony Forming Unit per Gram,LOD = Limit of Detection, (µg/g) = Microgram per Gram(ppm) =Parts per Million, (ppm) = (µg/g), (aw) = aw(area ratio) = Area Ratio, (mg/Kg) = Milligram per Kilogram